


**Donning instructions:**

Help the child don the cannula (with the tab pointing down so that the cannula nasal tips curve toward their head), then loop the cannula tubes over their ears as shown. Adjust the adjustment slider until a comfortable, secure fit is achieved.

**OR**

Loop the cannula over the child's head as shown so that the feed tube is behind them, then insert the cannula (with the tab pointing down so that the cannula nasal tips curve toward their head) and loop the cannula tubes back over their ears as shown. Adjust the adjustment slider until a comfortable, secure fit is achieved.

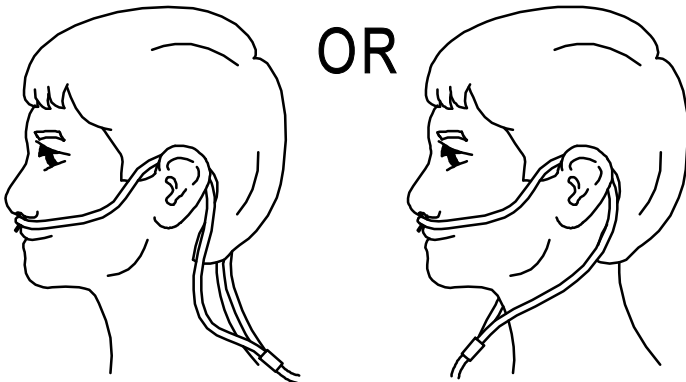

**Tab on cannula MUST point down towards lip**

51EDS-0006-00\$-


Made in the USA

**Donning instructions:**

Help the child don the cannula (with the tab pointing down so that the cannula nasal tips curve toward their head), then loop the cannula tubes over their ears as shown. Adjust the adjustment slider until a comfortable, secure fit is achieved.

**OR**

Loop the cannula over the child's head as shown so that the feed tube is behind them, then insert the cannula (with the tab pointing down so that the cannula nasal tips curve toward their head) and loop the cannula tubes back over their ears as shown. Adjust the adjustment slider until a comfortable, secure fit is achieved.

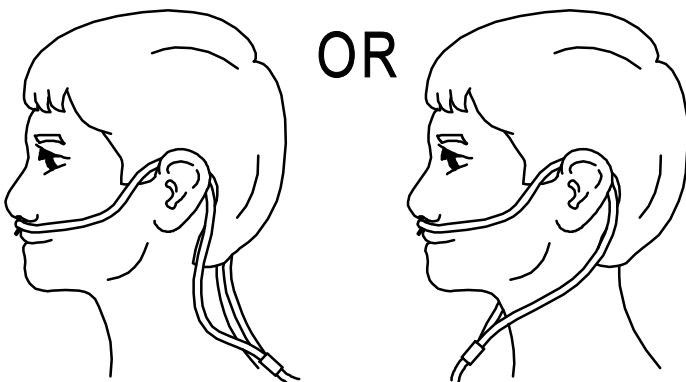

**Tab on cannula MUST point down towards lip**

51EDS-0006-00\$-


Made in the USA

**EDS STANDARD PEDIATRIC CANNULA**

00EDS-1086-00 (48") \_\_\_\_\_



EXPIRATION DATE STAMP

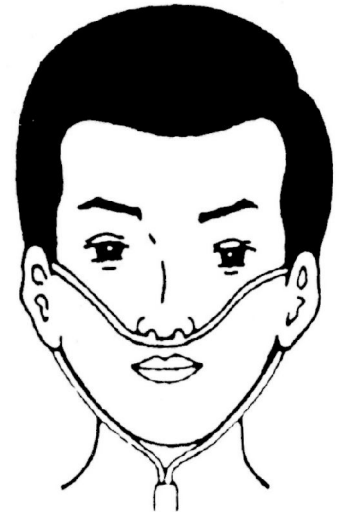


2244 SE Airport Way Suite 100, Redmond, Oregon 97756-7537 • 800-468-8185 • www.mhoxygen.com

**EDS STANDARD PEDIATRIC CANNULA**


00EDS-1086-00 (48") \_\_\_\_\_



EXPIRATION DATE STAMP

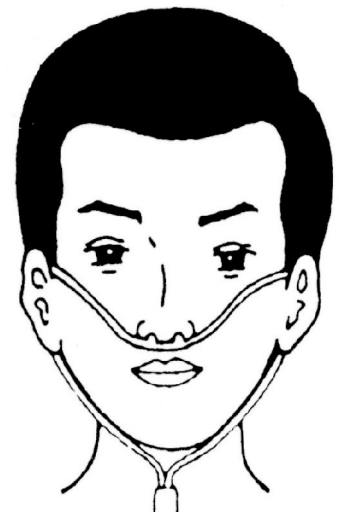


2244 SE Airport Way Suite 100, Redmond, Oregon 97756-7537 • 800-468-8185 • www.mhoxygen.com

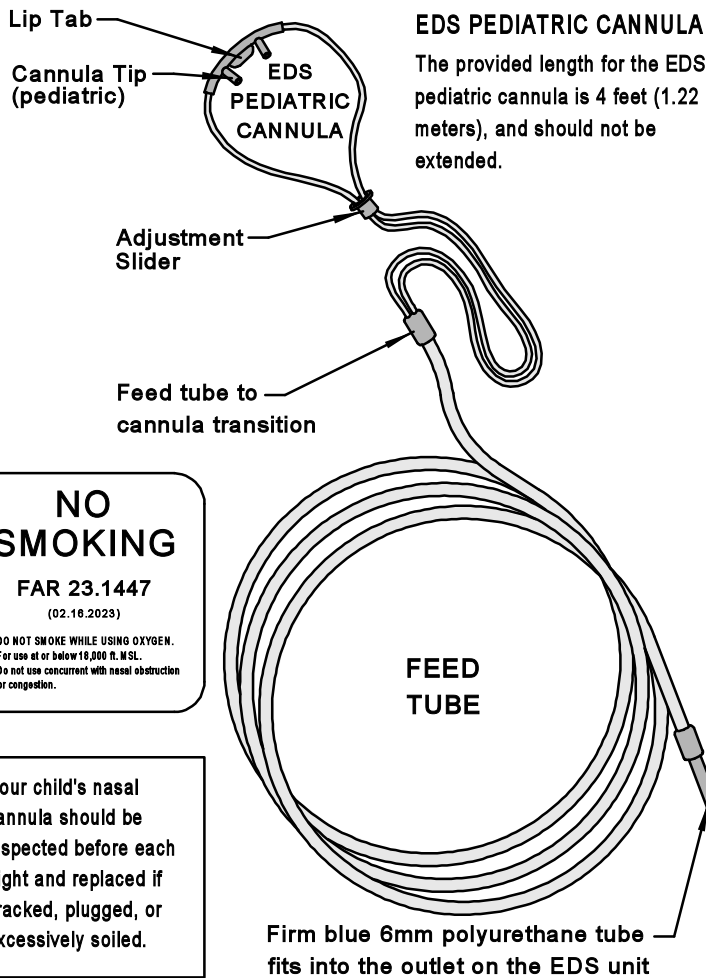

**IMPORTANT NOTE: The EDS Cannula is a personal device and for health reasons should not be shared between persons. In addition, it is the only item in the EDS system that should be replaced frequently, because even with the best cleaning efforts, bacteria and such can contaminate the cannula and pose a health risk.**

**Cannula cleaning instructions:**

- Create a solution of Milton™ (or equivalent) Sterilizing Fluid OR Tablets, & room-temperature water (follow Milton™ instructions to create solution).
- Soak the entire EDS cannula in the Milton™ solution for a minimum of 15 minutes (1 hour is preferred). Ensure the cannula is fully submerged and there is no air trapped in the tubing.
- Remove the cannula from the solution and remove excess solution still trapped in the cannula. This may be done by very gentle application of compressed air through the cannula from the EDS "blue" tube end. DO NOT mouth-blow through the EDS "blue" end or the entire cannula will need to be re-cleaned in the solution.
- Hang cannula and allow to air-dry in a clean, dry environment between 40°F and 95°F

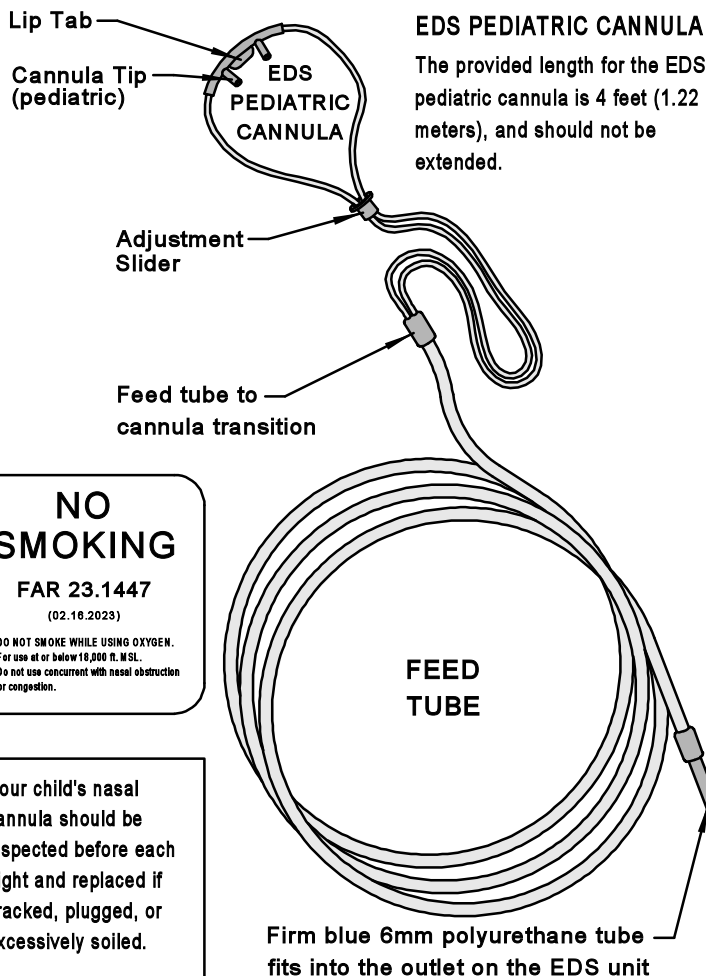

**IMPORTANT NOTE: The EDS Cannula is a personal device and for health reasons should not be shared between persons. In addition, it is the only item in the EDS system that should be replaced frequently, because even with the best cleaning efforts, bacteria and such can contaminate the cannula and pose a health risk.**

**Cannula cleaning instructions:**

- Create a solution of Milton™ (or equivalent) Sterilizing Fluid OR Tablets, & room-temperature water (follow Milton™ instructions to create solution).
- Soak the entire EDS cannula in the Milton™ solution for a minimum of 15 minutes (1 hour is preferred). Ensure the cannula is fully submerged and there is no air trapped in the tubing.
- Remove the cannula from the solution and remove excess solution still trapped in the cannula. This may be done by very gentle application of compressed air through the cannula from the EDS "blue" tube end. DO NOT mouth-blow through the EDS "blue" end or the entire cannula will need to be re-cleaned in the solution.
- Hang cannula and allow to air-dry in a clean, dry environment between 40°F and 95°F