


**Donning instructions:**

Help the child don the cannula (with the tab pointing down so that the cannula nasal tips curve toward their head), then loop the cannula tubes over their ears as shown. Adjust the adjustment slider until a comfortable, secure fit is achieved.

**OR**

Loop the cannula over the child's head as shown so that the feed tube is behind them, then insert the cannula (with the tab pointing down so that the cannula nasal tips curve toward their head) and loop the cannula tubes back over their ears as shown. Adjust the adjustment slider until a comfortable, secure fit is achieved.

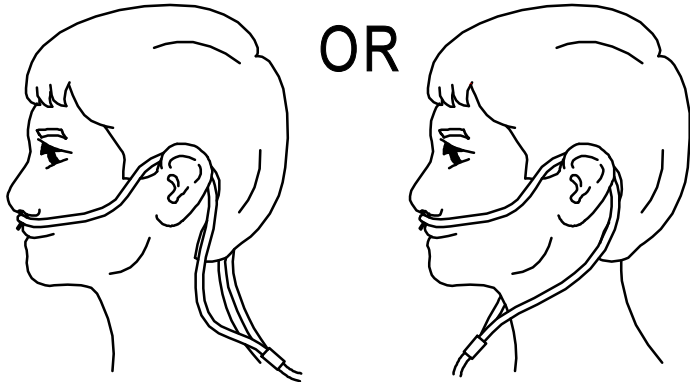

**Tab on cannula MUST point down towards lip**

51VEN-0065-00\$-


Made in the USA

**Donning instructions:**

Help the child don the cannula (with the tab pointing down so that the cannula nasal tips curve toward their head), then loop the cannula tubes over their ears as shown. Adjust the adjustment slider until a comfortable, secure fit is achieved.

**OR**

Loop the cannula over the child's head as shown so that the feed tube is behind them, then insert the cannula (with the tab pointing down so that the cannula nasal tips curve toward their head) and loop the cannula tubes back over their ears as shown. Adjust the adjustment slider until a comfortable, secure fit is achieved.

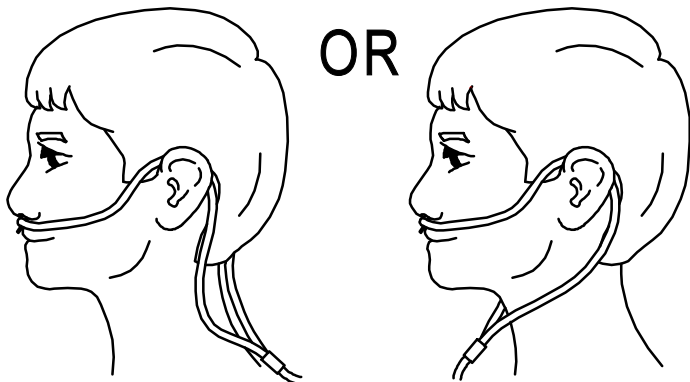

**Tab on cannula MUST point down towards lip**

51VEN-0065-00\$-


Made in the USA

**XCP STANDARD PEDIATRIC CANNULA**

00XCP-1045-00 (48") \_\_\_\_\_



EXPIRATION DATE STAMP

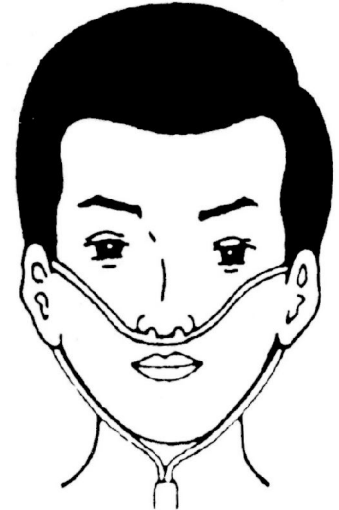


2244 SE Airport Way Suite 100, Redmond, Oregon 97756-7537 • 800-468-8185 • www.mhoxygen.com

**XCP STANDARD PEDIATRIC CANNULA**


00XCP-1045-00 (48") \_\_\_\_\_





EXPIRATION DATE STAMP

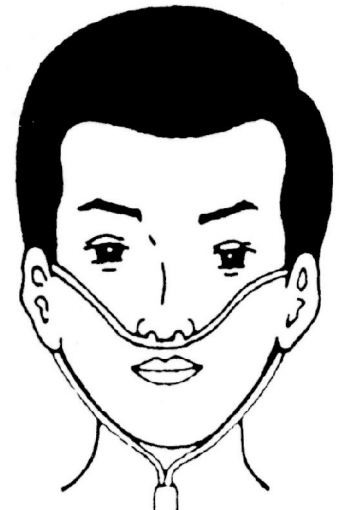

2244 SE Airport Way Suite 100, Redmond, Oregon 97756-7537 • 800-468-8185 • www.mhoxygen.com

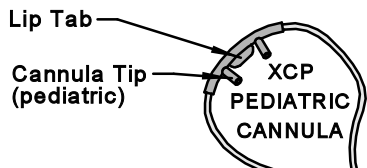

**XCP PEDIATRIC CANNULA**  
 The provided length for the XCP pediatric cannula is 4 feet (1.22 meters), and should not be extended.

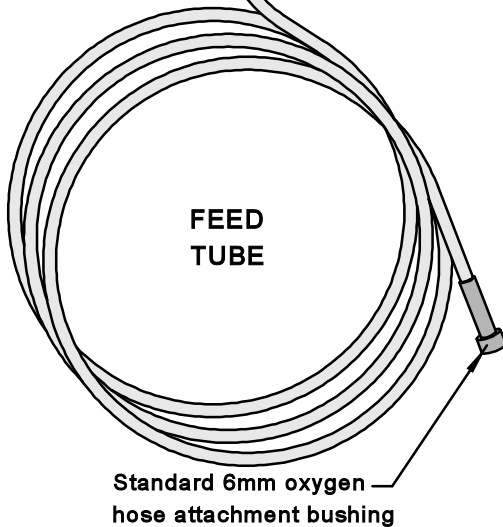

**NO SMOKING**  
 FAR 23.1447  
 (02.10.2023)  
 •DO NOT SMOKE WHILE USING OXYGEN.  
 •For use at or below 10,000 ft. MSL.  
 •Do not use concurrent with nasal obstruction or congestion.


Your child's nasal cannula should be inspected before each flight and replaced if cracked, plugged, or excessively soiled.

**IMPORTANT NOTE: The XCP Cannula is a personal device and for health reasons should not be shared between persons. In addition, it is the only item in the XCP constant-flow system that should be replaced frequently, because even with the best cleaning efforts, bacteria and such can contaminate the cannula and pose a health risk.**



Requires 1liter/minute per 10,000ft elevation.  
 Use with the MH-4 flowmeter only.

**Cannula cleaning instructions:**

- Create a solution of Milton™ (or equivalent) Sterilizing Fluid OR Tablets, & room-temperature water (follow Milton™ instructions to create solution).
- Soak the entire XCP cannula in the Milton™ solution for a minimum of 15 minutes (1 hour is preferred). Ensure the cannula is fully submerged and there is no air trapped in the tubing.
- Remove the cannula from the solution and remove excess solution still trapped in the cannula. This may be done by very gentle application of compressed air through the cannula from the oxygen hose attachment bushing (flowmeter) end. DO NOT mouth-blow through the flowmeter end or the entire cannula will need to be re-cleaned in the solution.
- Hang cannula and allow to air-dry in a clean, dry environment between 40°F and 95°F

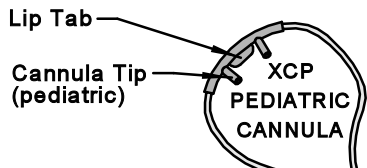

**XCP PEDIATRIC CANNULA**  
 The provided length for the XCP pediatric cannula is 4 feet (1.22 meters), and should not be extended.

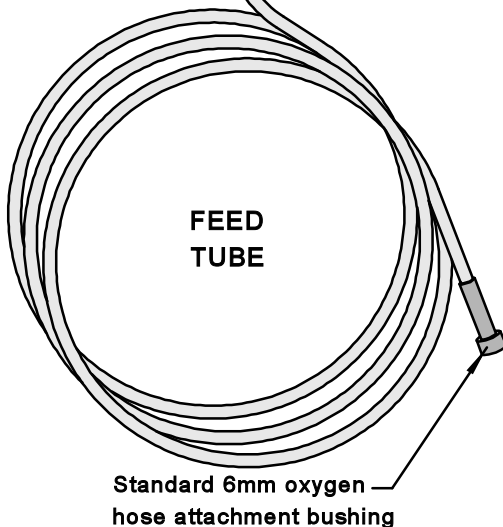

**NO SMOKING**  
 FAR 23.1447  
 (02.10.2023)  
 •DO NOT SMOKE WHILE USING OXYGEN.  
 •For use at or below 10,000 ft. MSL.  
 •Do not use concurrent with nasal obstruction or congestion.

Your child's nasal cannula should be inspected before each flight and replaced if cracked, plugged, or excessively soiled.

**IMPORTANT NOTE: The XCP Cannula is a personal device and for health reasons should not be shared between persons. In addition, it is the only item in the XCP constant-flow system that should be replaced frequently, because even with the best cleaning efforts, bacteria and such can contaminate the cannula and pose a health risk.**

Requires 1liter/minute per 10,000ft elevation.  
 Use with the MH-4 flowmeter only.

**Cannula cleaning instructions:**

- Create a solution of Milton™ (or equivalent) Sterilizing Fluid OR Tablets, & room-temperature water (follow Milton™ instructions to create solution).
- Soak the entire XCP cannula in the Milton™ solution for a minimum of 15 minutes (1 hour is preferred). Ensure the cannula is fully submerged and there is no air trapped in the tubing.
- Remove the cannula from the solution and remove excess solution still trapped in the cannula. This may be done by very gentle application of compressed air through the cannula from the oxygen hose attachment bushing (flowmeter) end. DO NOT mouth-blow through the flowmeter end or the entire cannula will need to be re-cleaned in the solution.
- Hang cannula and allow to air-dry in a clean, dry environment between 40°F and 95°F