



**Donning instructions:**

1. Place mask over your face covering both nose and mouth area, then slip elastic band over your head. The strap may be placed above or below your ears (see illustration below).
2. Adjust elastic band by pulling the band ends through the mask tabs until a comfortable, secure fit is achieved.
3. Pinch noseclip to provide a seal around the nose.
4. Attach the other end of the tubing with the CPC connector into the oxygen outlet and breathe normally.

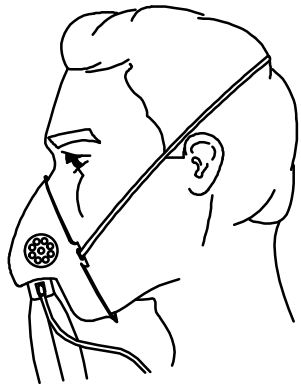

OR

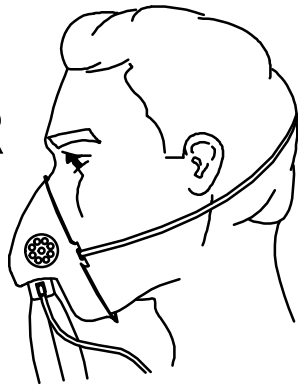

51EOS-0018-00\$-

Made in the USA


**EOS EMERGENCY OXYGEN  
SYSTEM FACEMASK**

00EOS-0018-00 (36") \_\_\_\_\_



EXPIRATION DATE STAMP


**MH**  
Aviation Oxygen Systems  
**MOUNTAIN HIGH**  
Equipment & Supply Company

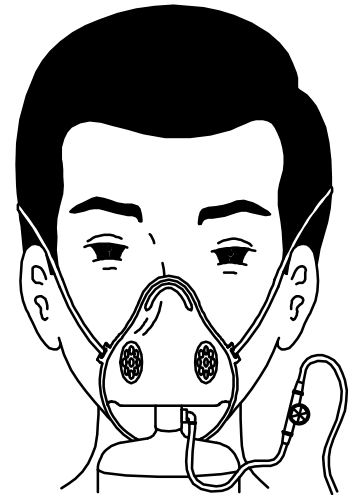


2244 SE Airport Way Suite 100, Redmond, Oregon 97756-7537 • 800-468-8185 • www.mhoxygen.com

**Donning instructions:**

1. Place mask over your face covering both nose and mouth area, then slip elastic band over your head. The strap may be placed above or below your ears (see illustration below).
2. Adjust elastic band by pulling the band ends through the mask tabs until a comfortable, secure fit is achieved.
3. Pinch noseclip to provide a seal around the nose.
4. Attach the other end of the tubing with the CPC connector into the oxygen outlet and breathe normally.

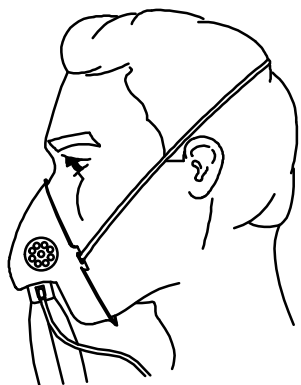

OR

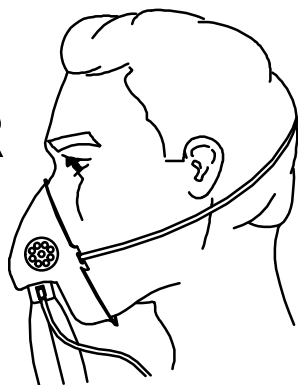


51EOS-0018-00\$-

Made in the USA


**EOS EMERGENCY OXYGEN  
SYSTEM FACEMASK**

00EOS-0018-00 (36") \_\_\_\_\_



EXPIRATION DATE STAMP

**MH**  
Aviation Oxygen Systems  
**MOUNTAIN HIGH**  
Equipment & Supply Company


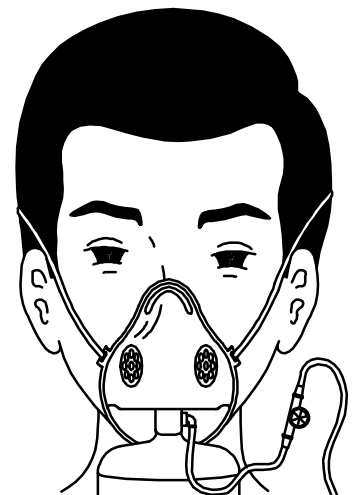


2244 SE Airport Way Suite 100, Redmond, Oregon 97756-7537 • 800-468-8185 • www.mhoxygen.com

**EOS EMERGENCY O2 FACE MASK**

Each EOS type face mask contains the following items:

- 1: CPC male snap quick-connector (w/ 3' feed tube).
- 2: Fixed flow control orifice (set to 3.0 liters/minute with an EOS regulator).
- 3: "Roto" type positive inline flow indicator.
4. Accumulating type non-rebreather face mask.

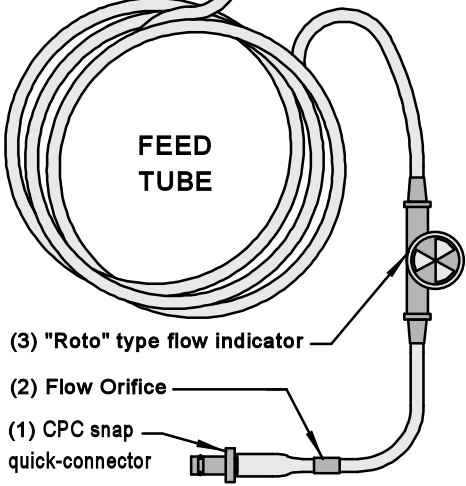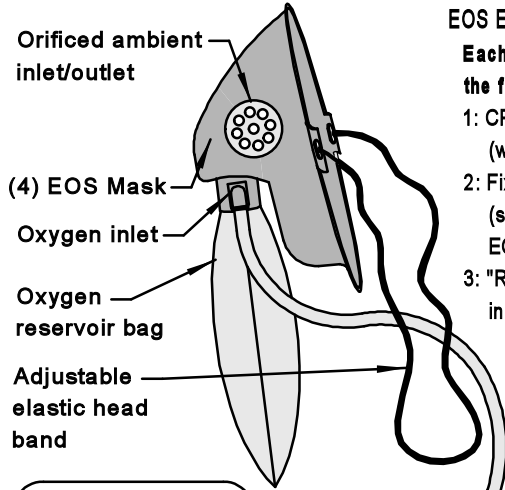

**NO SMOKING**  
 FAR 23.1447  
 (02.16.2023)  
 \*DO NOT SMOKE WHILE USING OXYGEN.  
 \*For use above or below 18,000 ft. MSL., not to exceed 30,000ft. MSL.


Your EOS face mask should be inspected before each flight and replaced if cracked, plugged, or excessively soiled.

**IMPORTANT NOTE: The EOS emergency O2 face mask is a personal device and for health reasons should not be shared between persons. In addition, the face mask is the only item in the EOS system that should be replaced periodically, because even with the best cleaning efforts, bacteria and such can contaminate the mask and pose a health risk.**

**Face mask cleaning instructions:**

After each use, wipe the facemask inside and outside with a cleaning wipe (MH p/n 00VEN-0077-00) or standard alcohol wipe. Hang facemask and allow to air-dry in a clean, dry environment between 40°F and 95°F. Ensure facemask is fully dry before use. Replace facemask when it becomes excessively soiled.

**Flow indicator:**





- Oxygen IS FLOWING if the flow indicator is SPINNING
- Oxygen is NOT FLOWING if it is NOT SPINNING

**EOS EMERGENCY O2 FACE MASK**

Each EOS type face mask contains the following items:

- 1: CPC male snap quick-connector (w/ 3' feed tube).
- 2: Fixed flow control orifice (set to 3.0 liters/minute with an EOS regulator).
- 3: "Roto" type positive inline flow indicator.
4. Accumulating type non-rebreather face mask.

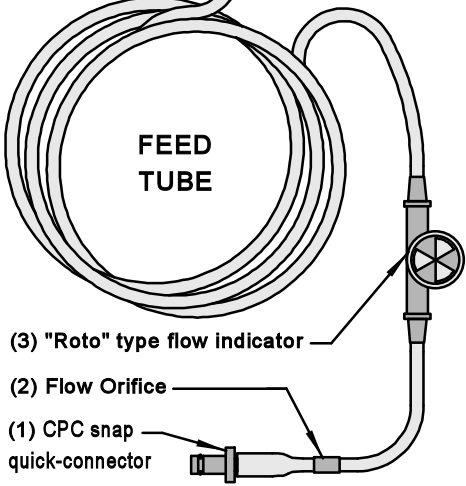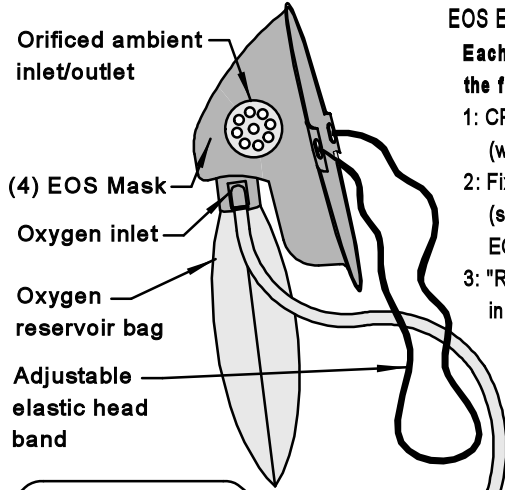

**NO SMOKING**  
 FAR 23.1447  
 (02.16.2023)  
 \*DO NOT SMOKE WHILE USING OXYGEN.  
 \*For use above or below 18,000 ft. MSL., not to exceed 30,000ft. MSL.

Your EOS face mask should be inspected before each flight and replaced if cracked, plugged, or excessively soiled.

**IMPORTANT NOTE: The EOS emergency O2 face mask is a personal device and for health reasons should not be shared between persons. In addition, the face mask is the only item in the EOS system that should be replaced periodically, because even with the best cleaning efforts, bacteria and such can contaminate the mask and pose a health risk.**

**Face mask cleaning instructions:**

After each use, wipe the facemask inside and outside with a cleaning wipe (MH p/n 00VEN-0077-00) or standard alcohol wipe. Hang facemask and allow to air-dry in a clean, dry environment between 40°F and 95°F. Ensure facemask is fully dry before use. Replace facemask when it becomes excessively soiled.

**Flow indicator:**



- Oxygen IS FLOWING if the flow indicator is SPINNING
- Oxygen is NOT FLOWING if it is NOT SPINNING